



Patents Office  
45 Merrion Square  
Dublin 2

I HEREBY CERTIFY that annexed hereto is a true copy of documents filed in connection with the following patent application:

Application No. S950163


Date of filing 1 March, 1995

Applicants SHANNON COOL LIMITED, an Irish Company  
of Bay 21, Shannon Industrial Estate,  
Shannon, County Clare, Ireland.

Dated this 4<sup>TH</sup> day of May, 1995

*V. Cunningham*

An officer authorised by the  
Controller of Patents, Designs and Trade Marks.

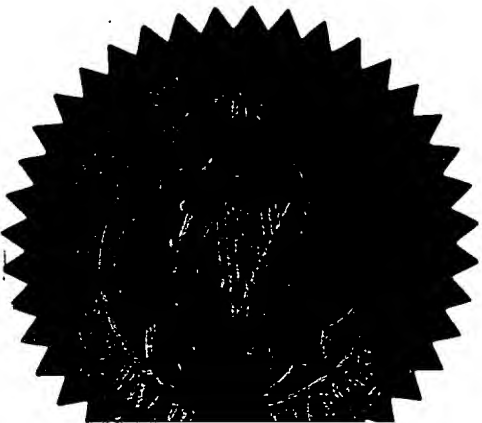

S 950163

FORM NO. 1

REQUEST FOR THE GRANT OF A PATENT

PATENTS ACT, 1992

The Applicants named herein hereby request  
\_\_\_\_\_ the grant of a patent under Part II of the Act  
\_\_\_\_\_ X the grant of a short-term patent under Part III of  
the Act  
on the basis of the information furnished hereunder.

1. Applicants

Name

SHANNON COOL LIMITED

Address

Bay 21,  
Shannon Industrial Estate,  
Shannon, County Clare,  
Ireland.

Description/Nationality

an Irish Company

2. Title of Invention

COLD THERAPY APPARATUS

3. Declaration of Priority on basis of previously filed  
application for same invention (Sections 25 & 26)

Previous filing date

Country in or for  
which filed

Filing No.

NONE

4. Identification of Inventor(s)

Names of persons believed  
by Applicants to be the inventors

1. PAUL THEODORE KOLEN; and 2. THOMAS D. FORD

Address

1. 139 Fourth Street, Encinitas, California 92024,  
United States of America; and
2. 10405 Orozco Street, San Diego, California 92124,  
United States of America.

CONTINUED OVER

5. Statement of right to be granted a patent (Section 17(2)(b))  
a Deed of Assignment dated February 10, 1995
6. Items accompanying this Request - tick as appropriate
- (i)   X   prescribed filing fee (£55.00)
- (ii)   X   specification containing a description and claims  
       specification containing a description only  
  X   Drawings referred to in description or claims
- (iii)   X   An abstract
- (iv)        Copy of previous application whose priority  
is claimed
- (v)        Translation of previous application whose  
priority is claimed
- (vi)        Authorisation of Agent (this may be given at 8  
below if this Request is signed by the Applicant)

## 7. Divisional Application

The following information is applicable to the present application which is made under Section 24 -

Earlier Application No: .....  
Filing Date: .....

8. Agent

The following is authorised to act as agent in all proceedings connected with the obtaining of a Patent to which this request relates and in relation to any patent granted -

Name

Address

F. R. KELLY & CO.

at their address as recorded for  
the time being in the Register of  
Patent Agents

9. Address for Service (if different from that at 8)

SHANNON COOL LIMITED  
BY: F. R. KELLY & CO.

Signed

Name :

Capacity

EXECUTIVE

Date

March 1, 1995

TRUE COPY  
AS  
LODGED

BACKGROUND OF THE INVENTION

1  
\$ 950 163  
APPLICATION No.

This invention relates to the application of cold or heat to affect heat transfer to or from the human or mammalian body. The necessity for such an application may arise in a wide range of circumstances. Most common are injuries, bruises, sprains, or other trauma to bone, muscle, ligaments, tendons, skin and other forms of mammalian tissue. The application of cold or cooling to reduce swelling, reduce pain and promote healing at the traumatized area of the human or mammalian body is often recommended. Similarly, the application of heat or heating to the human or mammalian body is used to warm up or "loosen-up" joint tissue such as ligaments or tendons prior to use to facilitate an increased range of motion prior to normal or strenuous physical activities.

Other circumstances in which the need for application of cold or heat therapy to the human or mammalian body may arise include post-surgical therapy to reduce pain and swelling and promote healing, as well as in orthopedic therapy, sports medicine therapy and rehabilitation programs and applications. Of particular importance are the areas of athletic injury and subsequent therapy, healing and rehabilitation in humans, and injury and subsequent therapy, healing and rehabilitation in thoroughbred race horses.

The most common method of achieving the desired cooling effect has been application of an ice bag to the desired therapy site. This method has several limitations. Ice bags can be cumbersome to apply, and in the case of animals, for example thoroughbred race horses, may be difficult to maintain on the therapy site. Ice bags can apply uneven cooling to the therapy site, are often difficult to contour to the area of the mammalian body to be treated, and the intensity of cooling is difficult to control. Often the application is either too cold, or not cold enough. A common ice bag has further limitations as well. As the ice melts, an ice bag may leak, causing inconvenience or more serious consequences. Finally, the static application of cold or cooling can become uncomfortable and unpleasant, usually resulting in the subject prematurely terminating the application before the full beneficial affect can be achieved.

A number of variations have been proposed to improve upon the ice bag or pack, but none fully addressed all of its shortcomings. For example, some have been known to use a bag of frozen peas (or other vegetables) as a substitute for an ice bag. The frozen peas allow more uniform cooling of the site, generally contour to the site better than a bag of ice cubes, and apply less severe cooling. Of course, this alternative has a number of drawbacks as well. A bag of frozen peas has limited available cooling capacity, and as with any bag, contouring to a part of the mammalian body such as the human knee can be difficult or impossible, resulting in uneven cold application.

Other variations on the basic ice bag or ice pack include a wrap or strap-on device which holds the source of cooling on the therapy site. These devices generally are designed for use on specific locations on the human body, and generally contour better to the therapy site and are held in place by means of belts or straps. These devices also have several shortcomings, however. Certain types have built-in reservoirs to provide a source of cooling, such as containers of frozen water. These devices must be kept frozen until ready to use, and once their cooling capacity is expired, they must be re-frozen before they can be used again. The intensity of cooling with these wrap or strap-on devices is also difficult to control, and they are capable of applying only static cooling to the site. There are also generally cumbersome, as the source of thermal cooling must be located entirely within the device and held at or on the therapy site.

Also available are chemical cold-packs comprised of two or more chemical substances stored separately in a flexible packet. When needed, the packet is manipulated, causing an internal seal to break and the chemical substances to mix. The substances, when mixed, have an endothermic reaction which causes the packet to cool. While these devices are useful in remote sites and in certain emergency situations, they afford little advantage over the ordinary ice bag. Furthermore, they can generally be used only one time, are of limited cooling capacity or duration,

operate at one non adjustable temperature, and are prohibitively expensive for use in a regular cold therapy program.

More recently, a commercially available apparatus for accomplishing the desired cooling of the human knee has been developed which incorporates a cold reservoir consisting of a large cooler. The water within the cooler is circulated by means of a pump which circulates the cooled water from the cooler through a tube to a bladder and back through a tube to the cooler. The bladder is applied to the therapy site and held in place by means of a wrap or strap device. This apparatus has many advantages over an ice pack or ice wrap. The cooler and source of cooling, generally ice, is held in a container separate from the therapy site. In this type of device, the rate of cooling is adjusted by increasing or decreasing the flow resistance by using a manually operated flow restriction valve or electrically setting the pump speed to a predetermined fixed value.

This apparatus also has several shortcomings. The device is incapable of supplying a measured and controlled cooling temperature to the therapy site, and is incapable of providing tactile stimulation to the therapy site. The device is also cumbersome in that the pump used to circulate the cooling fluid must be manually submerged in the cooler, and there is an ever-present danger of electrical shock due to the proximity of the electrical power cord and the circulating water.

The most common method for achieving the desired heating effect has been through the application of a hot water bottle or steamed towels to an injury site. As with similar cold therapy modalities, this form of heat therapy suffers from the same shortcomings in terms of ease of application and temperature regulation due to a lack of any temperature control mechanism at the injury site.



### DESCRIPTION OF THE PRIOR ART

Heretofore, a number of devices and systems have been employed to impose cold with or without pressure on parts of the human or mammalian body. Miller (US Patent No. 2,531,074 of November 21, 1950) discloses an appliance for a dry massage of a therapy site by water of controlled temperature in a sequence at alternatively high and low pressures applied to a multitude of adjacent chambers of flexible wall material and suggests that the water can be either heated or cooled.

Chessey (US Patent No. 2,726,658 of December 13, 1955) discloses a system, including a coolant control and supply unit, and a liquid-impervious appliance receiving the coolant and applied as a pad to a body portion of an animal, including a mechanical refrigeration system thermostatically controlled by the temperature of the coolant which is pumped through the appliance.

Grossan (US Patent No. 3,993,053 of August 5, 1975) discloses a massaging system including a flexible pad having fixed to one face a set of elastic tubing coils forming part of a recirculating hydraulic system, including a pump for creating pulsating fluid flow, and suggests that the pressure and temperature of the circulating liquid may be controlled by the operator.

Copeland, et al. (US Patent No. 4,149,529 of September 16, 1977) discloses a portable apparatus for controllably cooling and variably applying pressure to a portion of a mammalian body including a liquid supply, control unit, means to circulate the liquid and heat exchanger in the fluid reservoir mounted in a supply unit of sufficient size to support the weight of a human and receive a human limb such that the reservoir may be employed as a whirlpool bath.

Although all the devices described above may be functional and presumably operable, there is a need for an improved apparatus for applying cold or heat to a human or mammalian body which is small enough to be easily transported and used in a wide variety of locations, adaptable to many different mammalian body forms and potential therapy sites, capable of providing controlled temperature therapy at a preset temperature or by a pre-programmed temperature profile, capable of monitoring the therapy temperature directly at the therapy site, and capable of providing tactile stimulation to the therapy site to alleviate the problems of static cooling and enhance the beneficial effects of the cooling therapy. The present invention fulfills these needs, and further provides related advantages.

## SUMMARY OF THE INVENTION

The present invention provides an easily transportable apparatus for applying closed-loop temperature controlled cold or heat to a portion of the human or mammalian body. The apparatus comprises an insulated water reservoir within a sturdy housing, covered by a splash-proof lid, and is small enough to be easily situated in any convenient location for cold/heat therapy by the user. Within the reservoir housing but external to the reservoir is contained a self-priming fluid pump with a means of exchanging a measured portion of the re-circulation water with water from the reservoir to maintain the circulation water at a desired temperature. The pump is powered by a small mechanically integrated electric motor. Also contained in this area are the microprocessor-based temperature and pump/heat exchanger control electronics, and internal fluid tubing connections between the pump and the water reservoir, and between the pump and supply line connectors mounted on the housing. User controls and a temperature read-out display are also located on the reservoir housing.

The reservoir in the reservoir housing can accommodate crushed ice, ice cubes or a pre-formed freezable cold source, such as commonly used in portable coolers, and contains enough cooling capacity for generally all therapy applications. The reservoir may be easily recharged with additional ice if needed while therapy is continuing, and without the need for the subject to remove the bladder from the therapy site. For heat therapy, hot

water can be introduced into the reservoir or the reservoir fluid can be actively heated by an immersible heater to maintain a constant temperature for controlled heating applications.

The apparatus monitors the therapy temperature and produces an audible signal when the cold or heat source is exhausted and the apparatus is no longer able to maintain the desired therapy temperature within certain preset tolerances.

The fluid supply lines from the pumps are connected to self-sealing, "quick disconnect" connectors, allowing the user to quickly and conveniently attach and detach various bladder types for various therapy applications. The apparatus can also be adapted to support simultaneous use of multiple bladders fluidly connected in series for therapy at multiple sites, as in bilateral surgery applications. Connecting the bladder to the reservoir housing is a pair of fluid supply lines which are terminated at one end by the mating half of the "quick disconnect" connectors mounted in the reservoir housing.

The supply line pair is held together and encapsulated by a layer of insulating material, such as closed-cell polyurethane foam, making the entire tubing assembly water-tight, durable, flexible, and fully insulated to reduce the ambient heat load on the unit and enhance the comfort and ease of use of the therapy apparatus. The supply line assembly may be of various lengths to suit the particular therapy subject and application. The supply line

assembly may be permanently affixed to the bladder or attached by means of "quick-disconnect" connectors at its terminal end. Affixed within the supply line assembly is a pair of thermistors or other suitable temperature-sensing devices, one located in each of the pair of fluid supply lines at or near the quick disconnect mounted in the reservoir housing, the output of which is monitored by the control electronics to implement the closed-loop temperature control of the cold or heat therapy.

Various shapes and sizes of bladder are contemplated to accommodate the various therapy subjects, whether human or animal, and the various therapy sites of the mammalian body. All bladders will generally consist of two layers of flexible plastic or other material, completely sealed or welded at the edge or seam, and constructed to allow generous expansion and contraction in response to the varying pressure imposed by the pumps when applying tactile stimulation, and to ensure even distribution of circulation water or other fluid and the subsequent cooling/heating effect on the therapy site.

The bladder is generally held within a mating strap or wrap, depending upon the therapy subject and site. The strap or wrap may be a fabric or rubber type material, such as neoprene rubber, which is secured to the therapy site by means of belts, straps, "Velcro" fasteners. The strap or wrap, when fastened properly, holds the bladder firmly and evenly against the therapy site, while allowing expansion and contraction in response to the

pressure fluctuations created by the pump when applying tactile stimulation.

The apparatus maintains temperature control at the therapy site by a controlled dynamic mixing of cold/hot water from the reservoir with the re-circulation water returning from the bladder within the heat exchanger. By using the real-time temperature information generated by the temperature sensing devices, the microprocessor controls the rate of reservoir/re-circulation fluid mixing within the heat exchanger. This maintains the circulation water temperature, and thus the injury site bladder temperature. To ensure even temperature distribution at the therapy site or sites, particularly when multiple bladders are used in series, maximum flow rates and delivery pressure is maintained to minimize the difference between outgoing and returning water temperatures regardless of the heat load. To achieve tactile stimulation at the desired therapy temperature, the pump is periodically turned off for a brief interval to allow the pressure within the bladder to return to zero before turning the pump back on. This action causes the bladder to undergo a deflation/inflation cycle which in turn causes a tactile stimulation in the tissue directly in contact with the bladder. The microprocessor-based control electronics and associated operating program operate the pump accordingly to provide maximum flow of circulation fluid and impose periodic pressure variations on the bladder such that the desired temperature control and tactile stimulation are provided at the therapy site.

The present invention provides an important advance in cold/heat therapy of human and other mammalian subjects that improves ease of use and enhances therapy effectiveness. Other features and advantages of the present invention will be apparent from the following more detailed description of the preferred embodiment, taken in conjunction with the accompanying drawings, which illustrates, by way of example, the principles of the invention.

**BRIEF DESCRIPTION OF THE DRAWINGS**

Figure 1 is a schematic view of the apparatus as typically used by a human subject when applying cold therapy to the knee joint.

Figure 2 is a perspective view of the reservoir housing with portions removed or broken away to reveal internal structure.

Figure 3 is a schematic view of the insulated supply lines and bladder showing the internal structure of the bladder.

Figure 4 is a cross-sectional view of a bladder.



### DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

Referring initially to Figure 2, there is shown the reservoir housing 4 which includes a protective outer case 2, and inner ice reservoir 19 which is formed within the outer case 2 and open at the top, but otherwise leak-proof. The walls of the reservoir 19 are spaced within and apart from the walls of the outer case 2, the internal space thus formed around the inner reservoir 19 is filled with a thermal insulation 18. The bottom wall 3 of the reservoir 19 is also covered with thermal insulation 18, thus insulating the reservoir 19. The reservoir 19 is covered during operation of the apparatus using a lid 5 which is also thermally insulated and incorporates a seal which fits snugly in the opening of the reservoir 19 to prevent leakage caused by splashing during movement of the apparatus.

Within the space adjacent to the reservoir 19 and within the outer case 2 are mounted the pump/heat exchanger 13, electric motor 9, microprocessor-based control electronics 7. pressurized water from the pump/heat exchanger 13 is supplied to the outlet quick disconnect 11 with the return water routed to the air/water separator 15 via the return quick disconnect 12 through return tube 1. To maintain a closed system, air from the priming valve 14 is vented back to the reservoir 19 via vent tube 17, with air vented from the air/water separator 15 via vent tube 16. Closed loop control is affected by two thermistors 20 placed in the supply tube to the outlet quick disconnect 11.

Electrical power is supplied from a conventional AC wall outlet through power connector 10 and power leads connecting to the switching power supply electronics 8.

Mounted on the reservoir housing 4 are user-operated display/control electronics 6 with push-button controls for user input and a digital display for setting and monitoring therapy temperature and time.

Referring to Figure 3, the bladder supply line assembly 40 is attached to the reservoir housing 4 by the mating halves of the "quick-disconnect" supply line connectors 21 and 22, connecting a pair of flexible supply tubes 41 and 42 to the internal fluid supply tubes via quick disconnects 11 and 12. The flexible supply tubes 41 and 42 are encased in thermal insulation 43 which reduces ambient heat loads and provides a comfortable means of managing the supply line assembly 40 on the therapy subject. Various lengths for the supply line assembly 40 are contemplated depending upon the particular therapy subject and application.

The supply line assembly 40 may be permanently affixed to the bladder 60 or attached by means of additional "quick-disconnect" supply line connectors 48 and 49.

Referring to Figure 3, the bladder 60 may be permanently affixed to the supply line assembly 40 or attached by means of the mating halves of additional "quick-disconnect" supply line connectors 38

and 39. Various bladder shapes and sizes are contemplated for application on specific therapy sites, such as the human knee, ankle, or elbow, to sufficiently surround the therapy site to achieve optimal cold therapy results. The general structure of the bladder 60 is preferably two layers of flexible, weldable polymer or other suitable material 61, which are heat-welded or otherwise sealed completely around the outer seam of the bladder 62. Bladder supply tubes 63 and 64 are attached to the bladder 60 by means of a leak-proof seal 65. The bladder 60 may incorporate one or more internal seams 66 or internal walls (not shown), the function of which is to direct the flow of cooling fluid from the bladder supply tubes 63 and 64 uniformly through the bladder 60, and provide control over expansion of the bladder 60 in response to the higher periodic pressure imposed during tactile stimulation of the therapy site as illustrated in figure 4.

Referring to Figure 1, the bladder 60 is held on the therapy site preferably by means of a wrap 70 made of neoprene rubber or other suitable insulating, flexible material, which is shaped to hold the bladder 60 snugly on the therapy site but allow flexibility for expansion and contraction of the bladder 60 during tactile stimulation of the therapy site. The wrap is held in place preferably by means of "Velcro" fasteners which are attached or sewn onto the wrap 70 such that the wrap 70 can be adjusted by the particular user to fit snugly and comfortably.

The apparatus maintains therapy temperature control at the therapy site by pumping circulation water at a precisely determined temperature from the pump/heat exchanger 13 through the bladder 60 to achieve the desired preset therapy temperature or preprogrammed therapy temperature-time profile, as monitored by the thermistors 20. The reservoir 19, pump/heat exchanger 13, supply tubes 41 and 42, and bladder 60 form a fluid circuit in which fluid may flow in either direction. Net flow through the bladder 60 is achieved by creating a pressurized output flow via the pump/heat exchanger 13 with the spent water returning from the bladder 60 to the air/water separator and ultimately to the inlet side of the pump/heat exchanger 13. The pump/heat exchanger 13, under microprocessor control, continuously displaces a precise amount of re-circulation water with water from the constant temperature reservoir to precisely maintain the temperature of the circulation water exiting the pump/heat exchanger 13. The displaced re-circulation water is returned to the reservoir via the air/water separator 15 to maintain a constant volume in the circulation system. To ensure a uniform temperature distribution at the therapy site or sites, particularly when multiple bladders are used in series in post-bilateral surgery therapy, maximum flow rate and pressure through the circulation system is maintained.

To achieve tactile stimulation when this mode of operation is selected by the user, while maintaining the preset or preprogrammed therapy temperature, the pump/heat exchanger 13 is

periodically turned off for preprogrammed intervals to periodically allow the pressure in the bladder 60 to be cycled between zero and maximum. This imposed periodic pressure variation on the bladder 60 will provide tactile stimulation at the therapy site while maintaining the desired therapy temperature through the resulting deflation/inflation cycles in response to the pressure variations.

The control electronics 7 incorporate sufficient non-volatile electronic memory to allow storage, recall and implementation of a plurality of preprogrammed or user-programmed therapy temperature-time profiles, in addition to the operating program of the apparatus. In addition to the plurality of preprogrammed therapy temperature-time profiles contemplated to be provided with the apparatus, user-programming may be accomplished through the keys incorporated into the control/display electronics 6.

The present invention provides an easily transportable cold therapy apparatus providing closed-loop therapy temperature control and tactile stimulation of the therapy site which may be used by human and mammalian subjects and employed on various therapy sites. Other embodiments within the scope of the invention are feasible. For example, a device with dual pumps capable of bi-directional flow closed-loop temperature control and increased tactile stimulation is feasible. A dual pump device could implement closed-loop temperature control using analog control electronics in the form of a solid state thermostat with

the therapy site temperature selected with a mechanically operated device, such as a potentiometer in conjunction with a temperature read-out device. Increased tactile stimulation for a dual pump device could be achieved by engaging both pumps simultaneously, imposing momentary higher pressure on the bladder with no net fluid flow momentarily. Since many changes could be made in the above construction and many apparently widely different embodiments of this invention could be made without departure from the scope thereof, it is intended that all matter contained in the above description or shown in the accompanying drawings shall be interpreted as being illustrative only and not limiting.

CLAIMS

What is claimed is:

1. A transportable cold/heat therapy apparatus for applying cold/heat therapy to one or more therapy sites on the human or mammalian body comprising:

A means to select and set a constant therapy temperature;

A means to program and store one or more therapy temperature-time profiles;

A means to control the therapy temperature at a substantially constant value, or to follow with substantial accuracy a therapy temperature-time profile;

A means to measure and monitor with substantial accuracy the therapy temperature applied at the therapy site or sites;

A means to apply tactile stimulation at the therapy site or sites while controlling therapy temperature; and

A means to warn the user whenever the apparatus lacks sufficient cooling or heating capacity to control the therapy temperature at a constant value, or according to a therapy temperature-time profile, within a preset temperature tolerance value.

2. The apparatus of claim 1 wherein said means to select and set a constant therapy temperature includes microprocessor-based control electronics and associated operating program, connected to user-operated push-button controls and a digital display, said push-button controls and said digital display enabling the user to manually select and visually confirm a constant therapy temperature, said control electronics and associated operating program capable of storing and retrieving the constant therapy temperature for purposes of implementing closed-loop therapy temperature control.
3. The apparatus of claim 1 wherein said means to program and store one or more therapy temperature-time profiles includes microprocessor-based control electronics and associated operating program, connected to user-operated push-button controls and a digital display, said push-button controls and said digital display enabling the user to manually select and visually confirm a therapy temperature-time profile, said control electronics and associated operating program capable of storing and retrieving the therapy temperature-time profile and determining the time-varying therapy temperature specified in the therapy temperature-time profile in real time for purposes of implementing closed-loop therapy temperature control.



4. The apparatus of claim 1 wherein said means to control the therapy temperature at a substantially constant value, or to follow with substantial accuracy a therapy temperature-time profile, includes microprocessor-based control electronics and associated operating program, said control electronics and associated operating program connected to said means to measure and monitor with substantial accuracy the therapy temperature applied at the therapy site or sites and having the capability of comparing the therapy temperature applied at the therapy site or sites to a constant therapy temperature, or to a time-varying therapy temperature specified in a therapy temperature-time profile in real time, for purposes of implementing closed-loop therapy temperature control, said control electronics also connected to the electric-powered fluid pump/heat exchanger. The fluid pump/heat exchanger having its fluid input connected to a reservoir containing cooled/heated fluid and the returning circulation water. The mixing of the reservoir and returning water is controlled via the control electronics to provide output water at a constant selected temperature. The controlled temperature fluid output is connected to the bladder device via the supply tubes having the capability of pumping fluid from said heat exchanger to said bladder device when operated.
5. The apparatus of claim 1 wherein said means to measure and monitor with substantial accuracy the therapy temperature

applied at the therapy site or sites includes microprocessor-based control electronics and associated operating program and two thermistors connected to said control electronics, one said thermistor mounted in each of two supply tubes supplying circulating fluid to a bladder device, said control electronics and associated operating program monitoring the output of said thermistors and computing the actual circulation fluid temperature detected by said thermistors for purposes of implementing closed-loop therapy temperature control via the pump/heat exchanger.

6. The apparatus of claim 1 wherein said means to apply tactile stimulation at the therapy site or sites includes a electric-powered fluid pump, said fluid pump connected to microprocessor-based control electronics and associated operating program, said fluid pump having its fluid input connected to a heat exchanger containing controlled temperature fluid and its fluid output connected by a fluid supply tube to a bladder device, and having the capability of pumping fluid from said heat exchanger to said bladder device when operated, said control electronics and associated operating program periodically modulates the bladder pressure for preprogrammed intervals, thereby periodically imposing near zero pressure on said bladder device thus creating tactile stimulation through the inflation/deflation cycle.

7. The apparatus of claim 1 wherein said means to warn the user whenever the apparatus lacks sufficient cooling/heating capacity to control the therapy temperature at a constant value, or according to a therapy temperature-time profile, within a preset temperature tolerance value includes two thermistors connected to microprocessor-based control electronics and associated operating program, one said thermistor mounted in each of two supply tubes supplying controlled temperature fluid to a bladder device, said control electronics and associated operating program monitoring the output of said thermistors and producing an audible signal from a sound-emitting device when the temperature detected by said thermistors indicates that the cooling/heating capacity in said reservoir is insufficient for maintenance of the closed-loop therapy temperature control within the preset temperature tolerance value.

### ABSTRACT OF THE DISCLOSURE

An apparatus for applying closed-loop temperature controlled cold and heat therapy, with or without tactile stimulation, to an injured or otherwise traumatized part of the human or mammalian body. The apparatus comprises an easily transportable unit containing the insulated water reservoir, an integrated pump/heat exchanger powered by a small electric motor, microprocessor-based electronic temperature and fluid controls, and a pair of insulated fluid supply lines connected to a sealed bladder which is applied on or at the therapy site and held in place by means of a strap or wrap device. The cold/heat therapy is applied by re-circulating water from the heat exchanger through the bladder and back to the heat exchanger at a fixed rate which maintains the bladder at a constant temperature regardless of the heat load presented by the therapy site. The desired therapy temperature may be preset by the user or programmed to follow a desired therapy temperature profile. Therapy temperature is monitored by internal thermistors located in each of the fluid supply lines. The microprocessor-based control electronics monitor the thermistor output and control the pump/heat exchanger to maintain the preset therapy temperature or follow the pre-programmed therapy temperature profile. Tactile stimulation of the therapy site is created while maintaining the desired temperature at the therapy site by controlling the pump pressure such that the fluid pressure imposed upon the bladder varies in a cyclical manner, causing the bladder to expand and contract thereby creating

tactile stimulation, while maintaining the desired temperature at the therapy site via the heat exchanger. The tactile stimulation greatly increases the comfort of the cold therapy, thereby promoting longer and more beneficial therapy sessions. When used for cold therapy, the water or other fluid in the reservoir, which is mixed with the re-circulation water via the heat exchanger under control of the microprocessor, may be cooled using a multitude of mediums, such as block ice, ice cubes, crushed ice, sealed re-usable cold sources, or other readily available cold source. Similarly, when used for heat therapy, the reservoir fluid may be pre-heated externally before being placed in the reservoir or be actively heated via an immersible heater separate from the main unit. The therapy unit may be connected to a multitude of bladder shapes and designs for various therapy applications, or multiple bladders fluidly connected in series. The bladders are designed to accommodate substantial expansion and contraction in response to the varying pressures imposed by the pump to enhance the magnitude of tactile stimulation.

PORTABLE COLD THERAPY UNIT

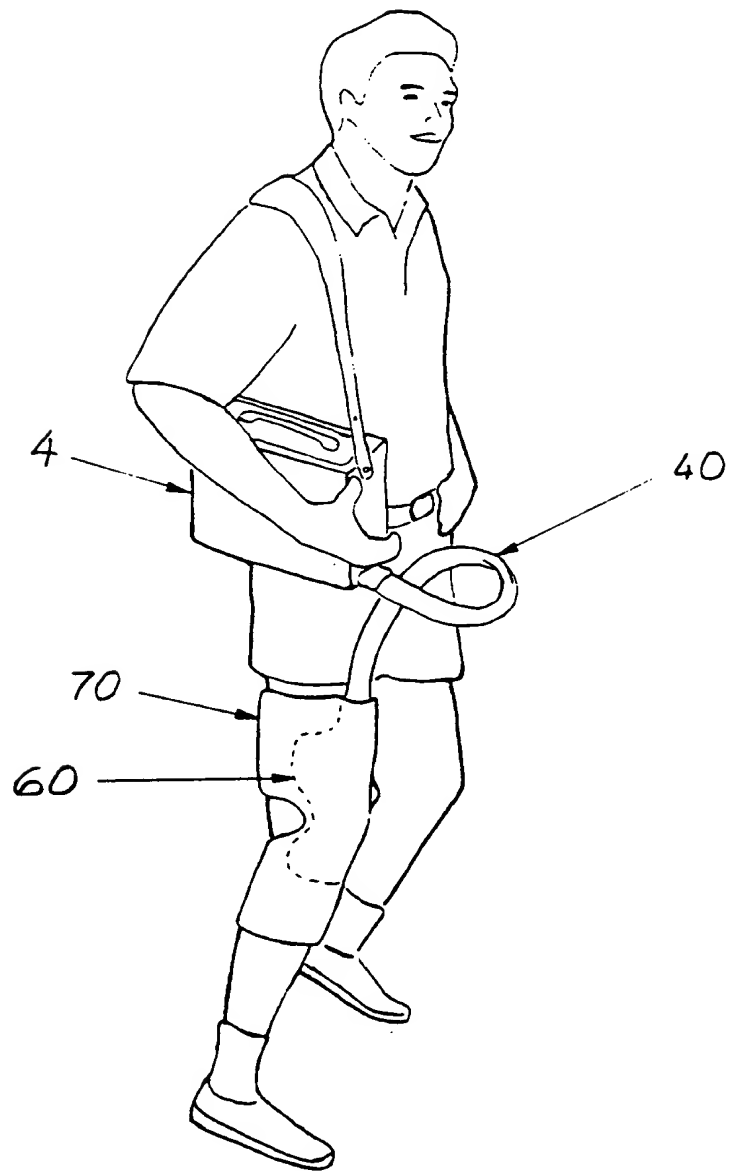
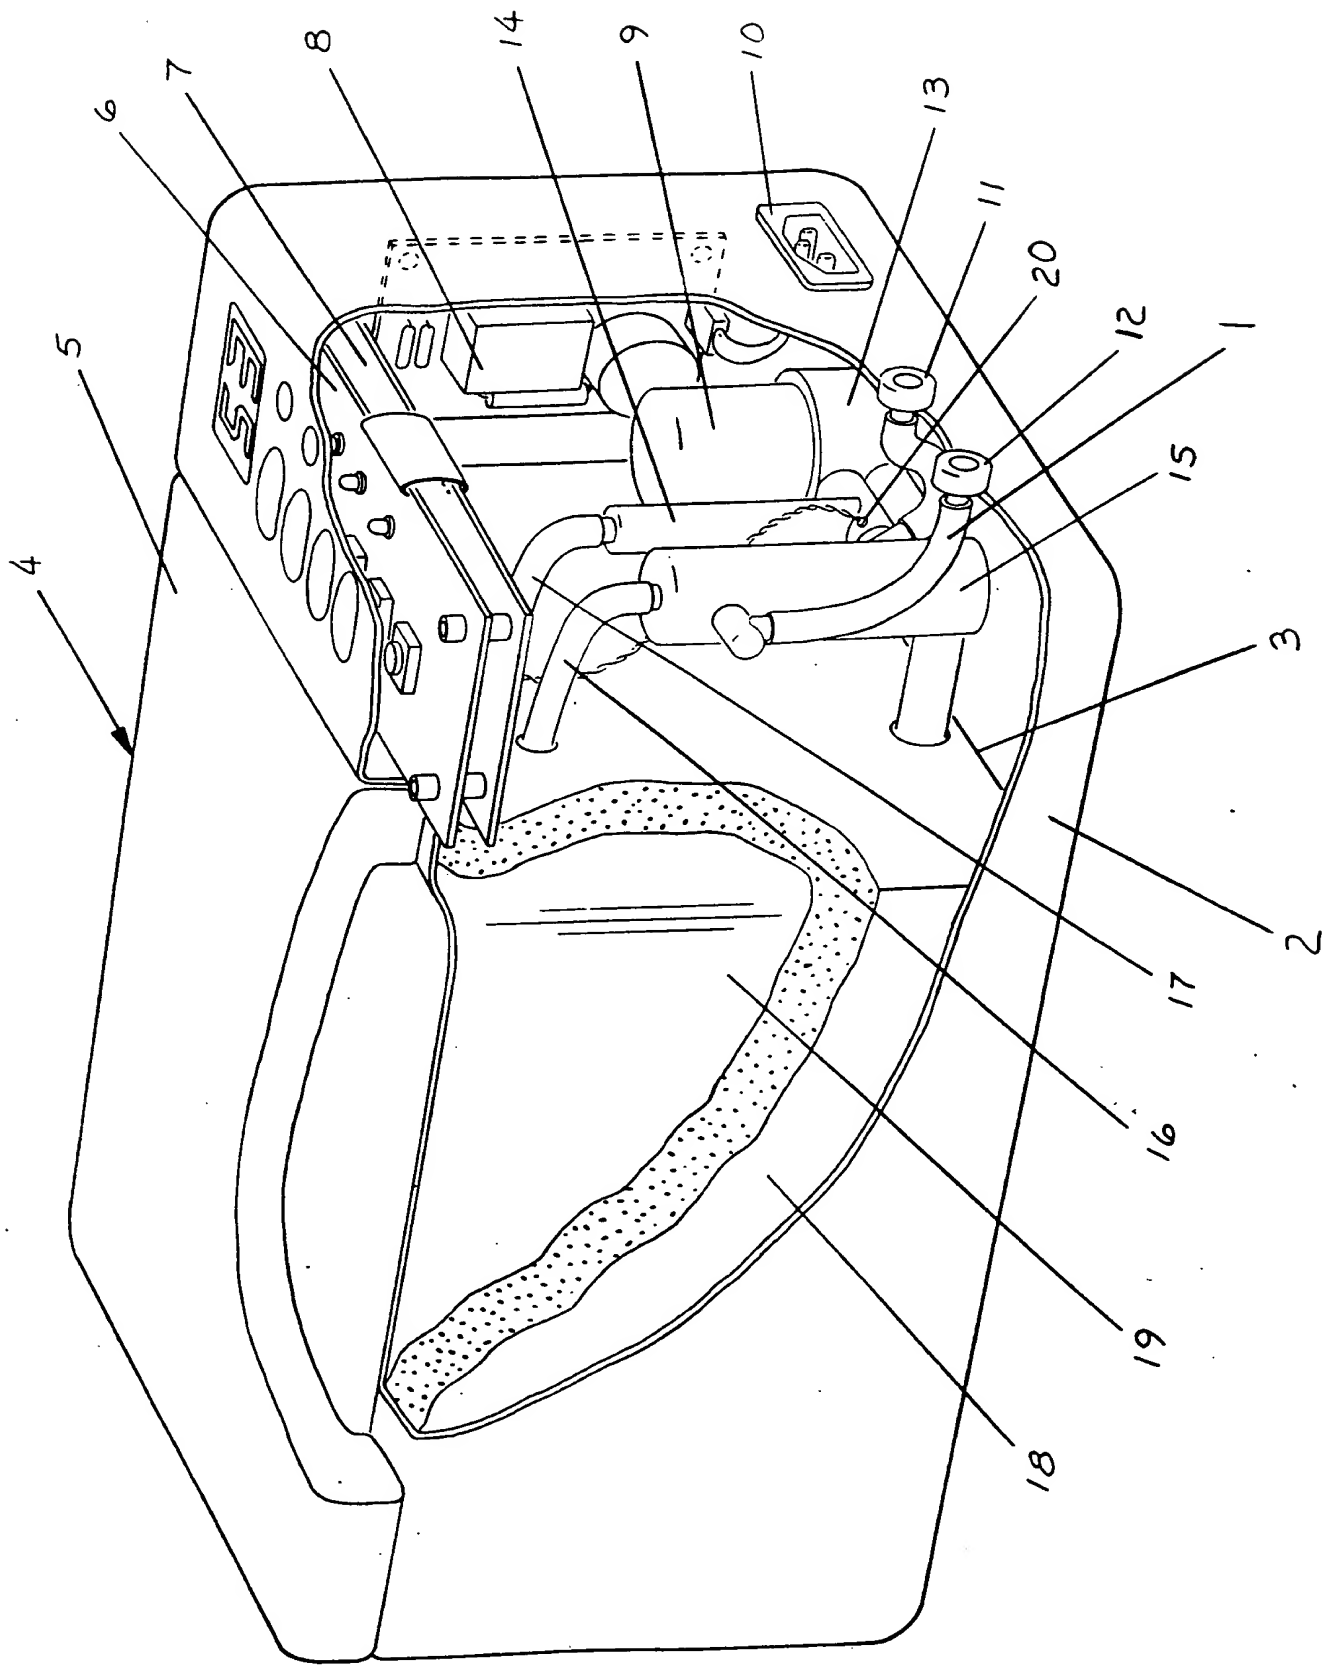
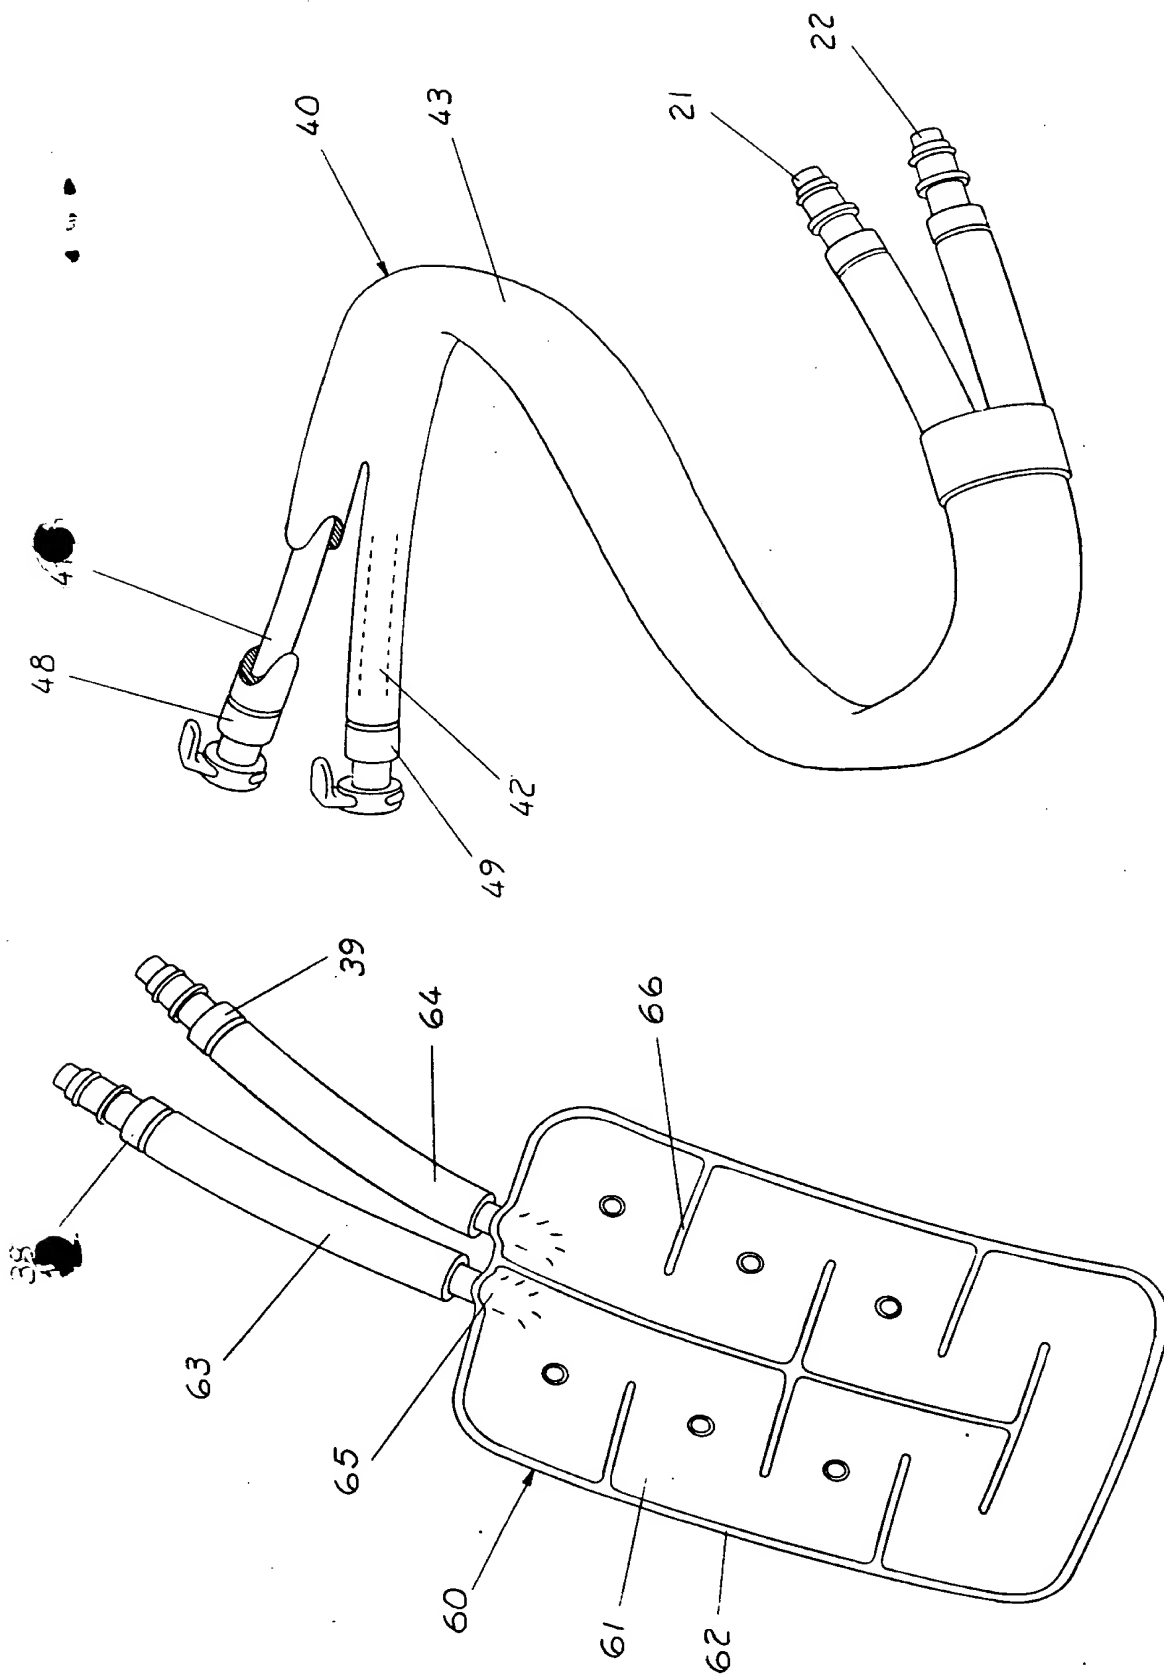


FIG. 1

Fig. 2







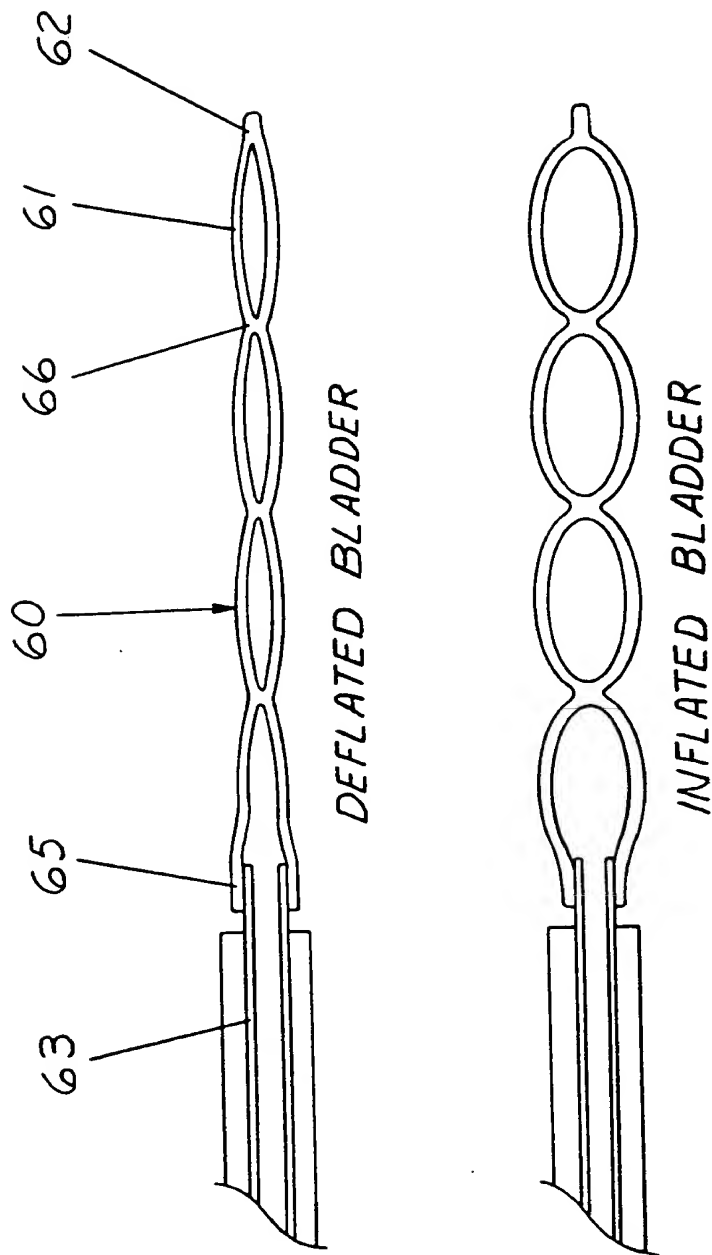


FIG. 4